

BT-08 SD3 DIAG 3032 FW:1.75.00D0
Aut


16/09/2025 10:57:10

10mm/s
20mm/mV
50Hz ADS 1.5s

HR = 69


HR = 69

HR = 69

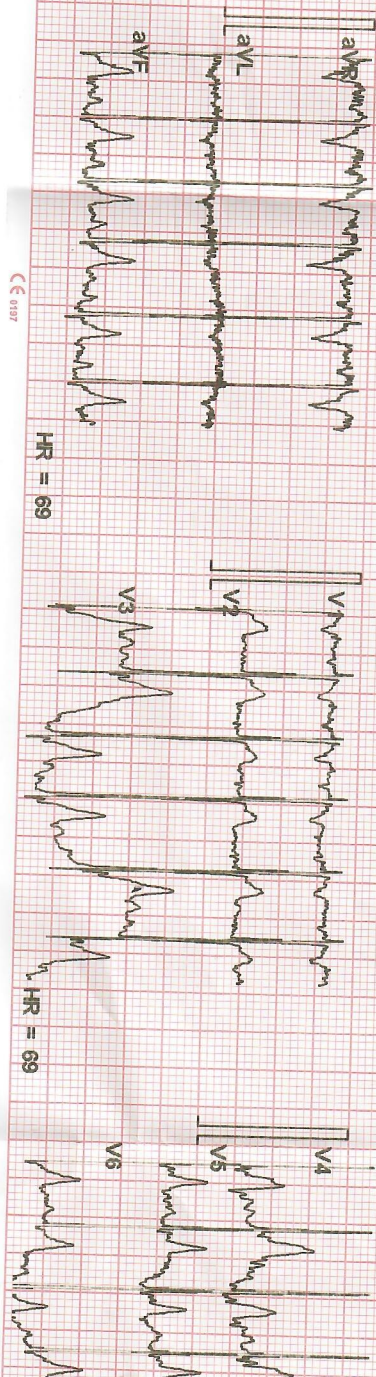

P.	Q	R	S	R'	S'	T+	T-	ST	STs [uV/s]	SF	74 t/min
-	-	281	-91	-	-	132	-	7	294	RR	816 ms
-	-	1582	-65	-	-	395	-	45	693	P	140 ms
-	-	1300	-47	-	-	259	-	34	384	QRS	104 ms
-	-	45	-	-	-	-	-	-261	-22	QT	158 ms
-	-	-	-	-	-	-	-	-10	-28	QTc	368 ms
-	-	-	-	-	-	-	-	37	574	axis P	407 ms
-	-	-	-	-	-	-	-	13	-312	axis QRS	70°
-	-	-	-	-	-	-	-	38	112	axis T	82°
-	-	-	-	-	-	-	-	29	2845		
-	-	-	-	-	-	-	-	16	480		
-	-	-	-	-	-	-	-	70	186		
-	-	-	-	-	-	-	-	12	621		


 ELARGISSEMENT ONDE P
 ECG NORMAL
 RYTHME SINUSAL


 J. B. Luey