

BTL-08 SD3 DIAG 3032 FW:4.75.0000
Aut


12/03/2024 08:46:44

25mm/s
10mm/mV
50Hz ADS 1.5s


HR = 60

CE 0187


CE 0187

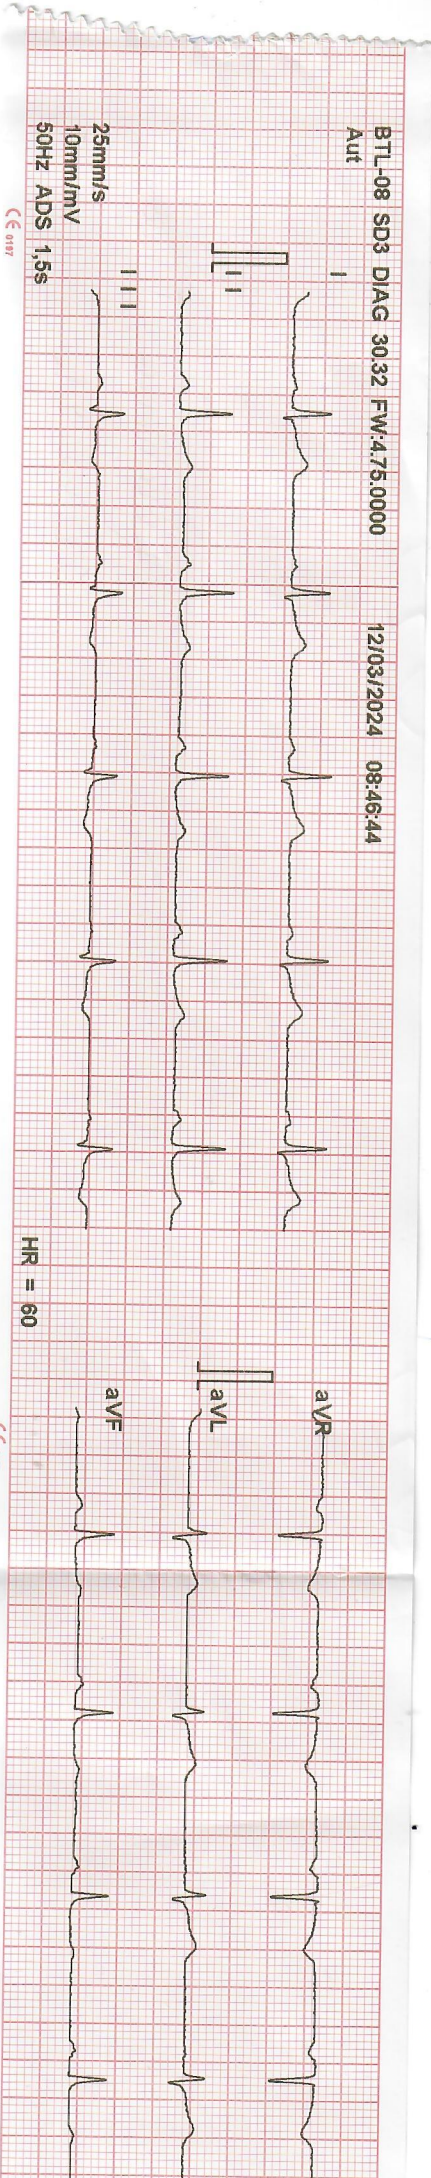


HR = 60

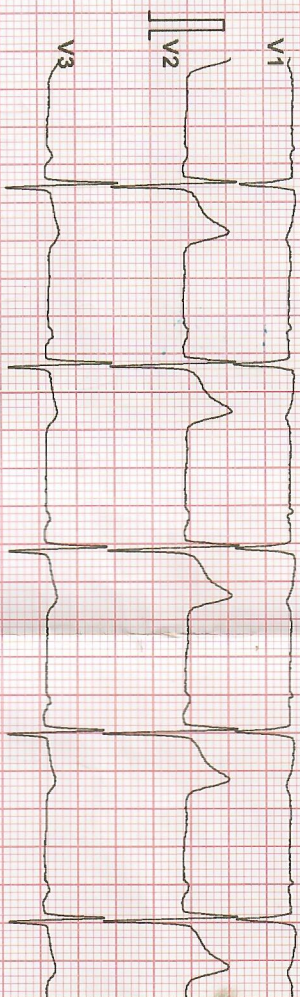

HR = 60

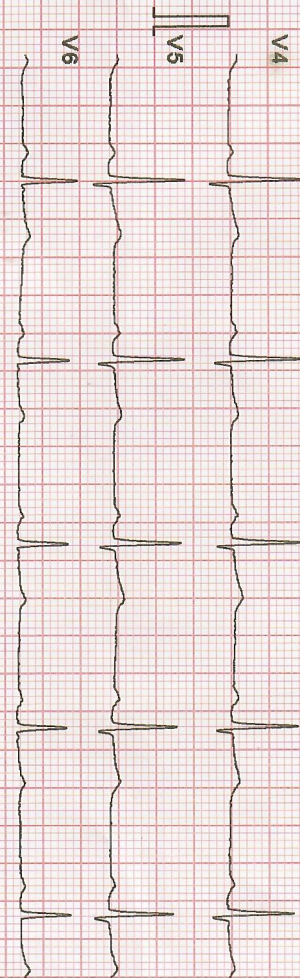

P	Q	R	S	R'	S'	T+	T-	ST	STs	SE	60 l/min
-	-	511	-124	-	-	193	-	9	442	RR	994 ms
-	-	717	-	-	-	127	-	15	73	P	94 ms
-	-135	347	-	-	-	-	-93	-1	-350	QRS	98 ms
-79	-603	264	-200	-	-	-	-164	-12	-273	QT	168 ms
-	-	480	-	-	-	141	-	4	406	QTc	388 ms
-	-715	-	-	-	-	47	-12	7	-124	axis P	389 ms
-	-	762	-1045	-	-	-	-47	39	-64	axis QRS	34°
-	-	827	-476	-	-	618	-	127	1341	axis T	0°
-	-	914	-196	-	-	158	-	53	464		
-	-	905	-192	-	-	120	-	23	221		
-	-	688	-	-	-	122	-	14	262		
-	-	-	-	-	-	101	-	9	127		

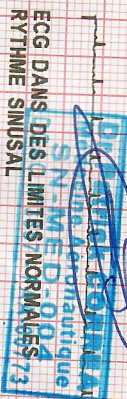

 ECG DANS DES LIMITES NORMALES

Ibrahim T. Huan

11-03-21