



BTL-08 SD3 DIAG 3032 FW4.75.0000  
Aut 28/03/2024 11:40:50


25mm/s  
10mm/mV  
50Hz ADS 1.5s

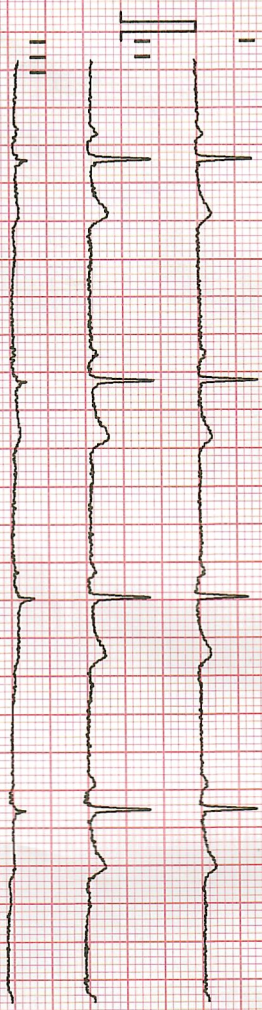

HR = 52

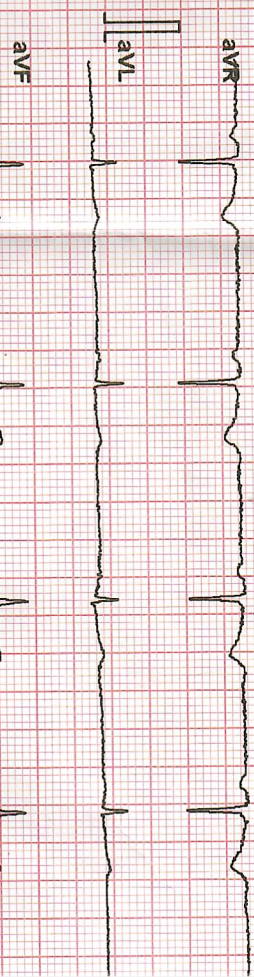

HR = 52  
C6 007

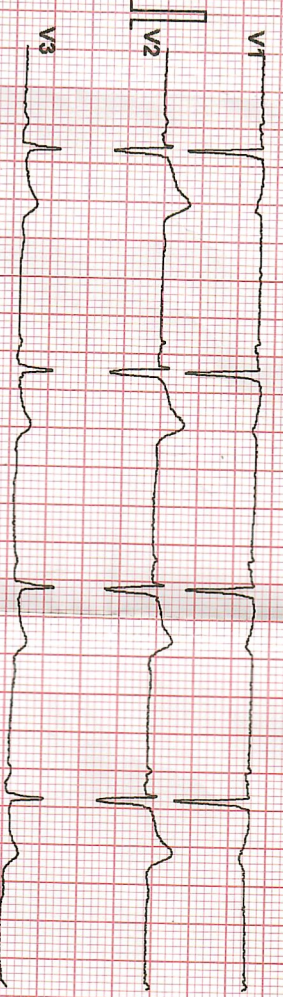


HR = 52

C6 007





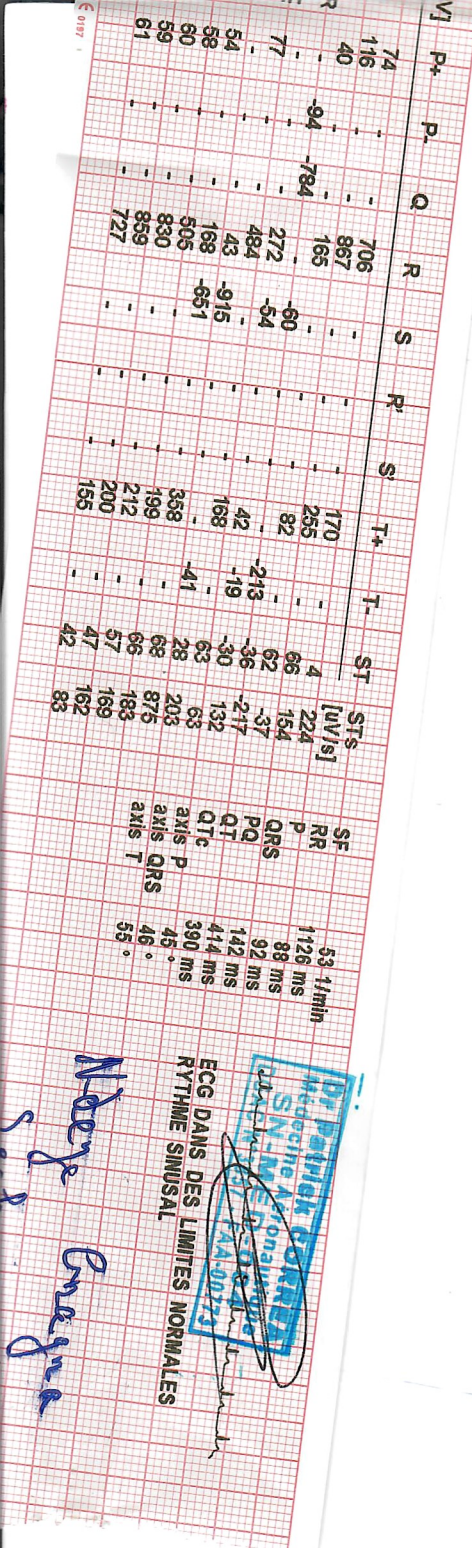

Dr. Patrick G. G. G. G.  
 Médecin A. G. G. G.  
 SN-ME-A-00273  
 ECG DANS DES LIMITES NORMALES  
 RYTHME SINUSAL

Alberge Enquête  
 5.1.9