

# Pure tone audiometry




Operator :PATRICK CORREA

Patient **MOR SAMBA DIOP**


Date of Birth 18 May 1976

Measurement date 23/01/2025 09:20:35

**Right**

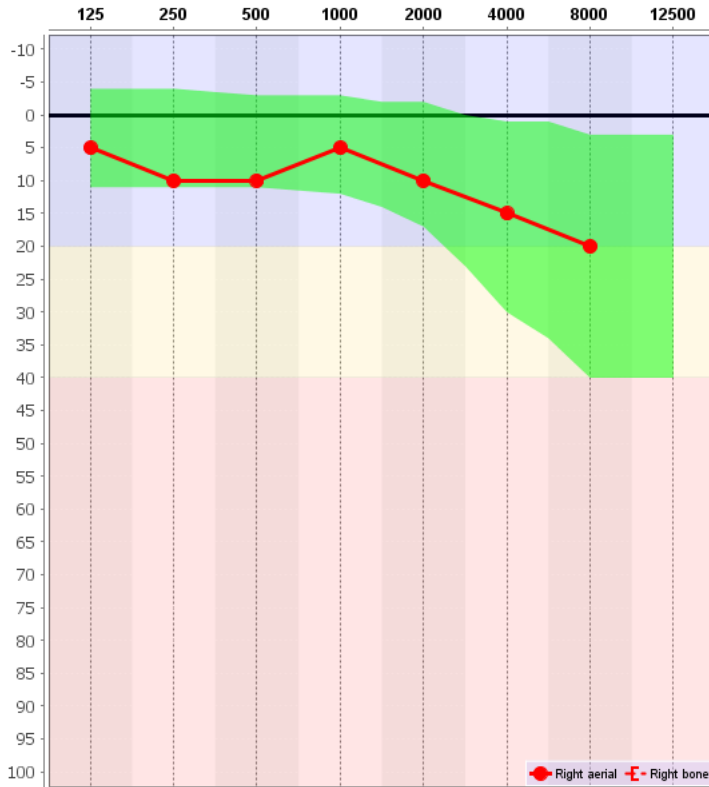

**Left**

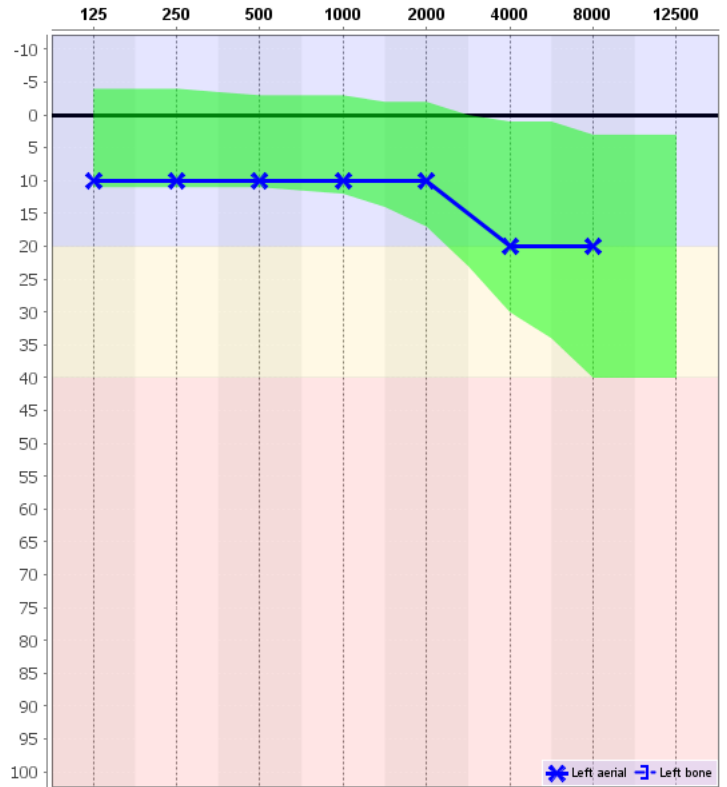

|                                                                              |             |                                                                    |        |             |        |        |        |
|------------------------------------------------------------------------------|-------------|--------------------------------------------------------------------|--------|-------------|--------|--------|--------|
|                                                                              | 500Hz       | 1000Hz                                                             | 2000Hz | 3000Hz      | 4000Hz | 6000Hz | 8000Hz |
| Left :                                                                       | 10 dB       | 10 dB                                                              | 10 dB  | N/C         | 20 dB  | N/C    | 20 dB  |
| Result: 1+2+3+4+6                                                            |             | Total = N/C                                                        |        |             |        |        |        |
| Unilateral Result: 1+2+3+4                                                   | (A)         | Total = N/C                                                        |        |             |        |        |        |
| Rapid Hearing Loss: 3+4+6 (compare to previous result; refer >=30dB differ.) |             |                                                                    |        | Total = N/C |        |        |        |
| Right :                                                                      | 10 dB       | 5 dB                                                               | 10 dB  | N/C         | 15 dB  | N/C    | 20 dB  |
| Result: 1+2+3+4+6                                                            |             | Total = N/C                                                        |        |             |        |        |        |
| Unilateral Result: 1+2+3+4                                                   | (B)         | Total = N/C                                                        |        |             |        |        |        |
| Rapid Hearing Loss: 3+4+6 (compare to previous result; refer >=30dB differ.) |             |                                                                    |        | Total = N/C |        |        |        |
| Difference between (A) & (B)                                                 | N/C         | >40dB is a unilateral loss (needs referral for any unknown issues) |        |             |        |        |        |
| Result Category:                                                             | Right = N/C |                                                                    |        | Left = N/C  |        |        |        |
| HSE Categorisation                                                           | N/C         |                                                                    |        |             |        |        |        |

Notes

Device used for the measurement  
 Device : OtoWin  
 S/N : 20605 - 014  
 Firmware : : 1.2.0e  
 Hardware : elios3  
 Stimulator : DD45 HI  
 Calibration date : 02/03/2020