


BTI-08 SD3 DIAG 3032 FW:4.75.0000
Aut


Age:0 Sexe:Masculin 13/06/2023 09:06:31 Médecin CORREA

25mm/s
10mm/mV
50Hz ADS 1.5s

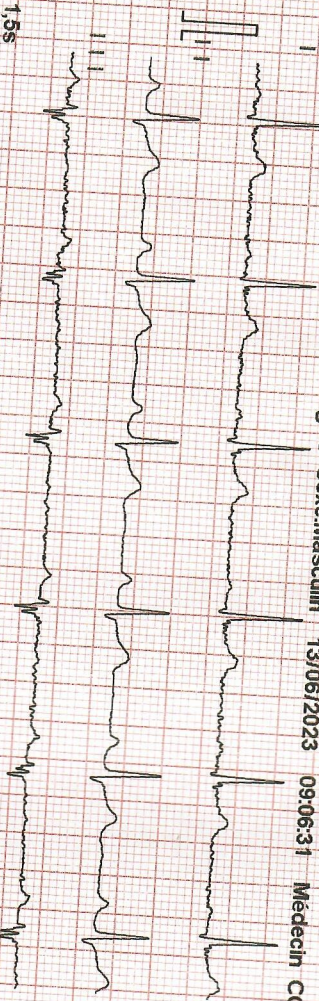

HR = 68


aVR
aVL
aVF

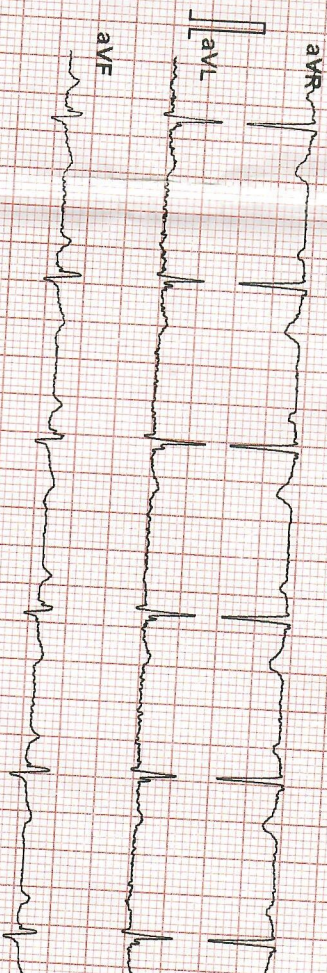


BTI-08 SD3 DIAG 30.32 FW:4.75.0000
Aut

Age:0 Sexe:Masculin 13/06/2023 09:06:31 Médecin CORREA

25mm/s
10mm/mV
50Hz ADS 1.5s

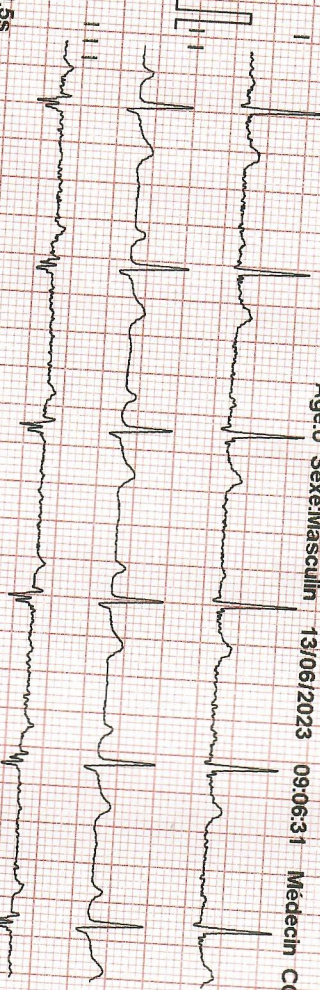


HR = 68

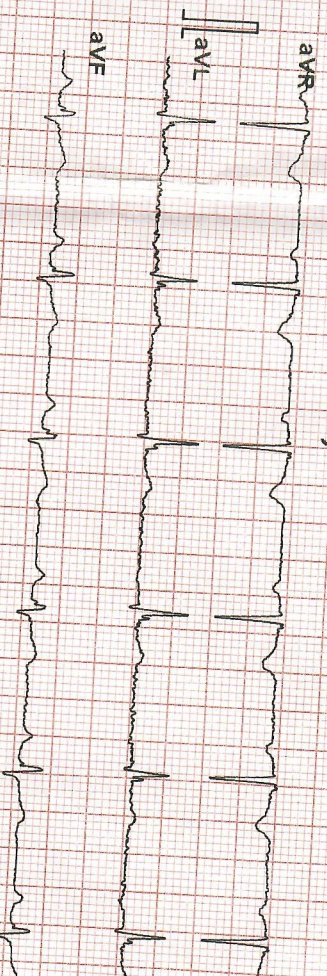

BTI-08 SD3 DIAG 30.32 FW:4.75.0000
Aut

Age:0 Sexe:Masculin 13/06/2023 09:06:31 Médecin CORREA

25mm/s
10mm/mV
50Hz ADS 1.5s

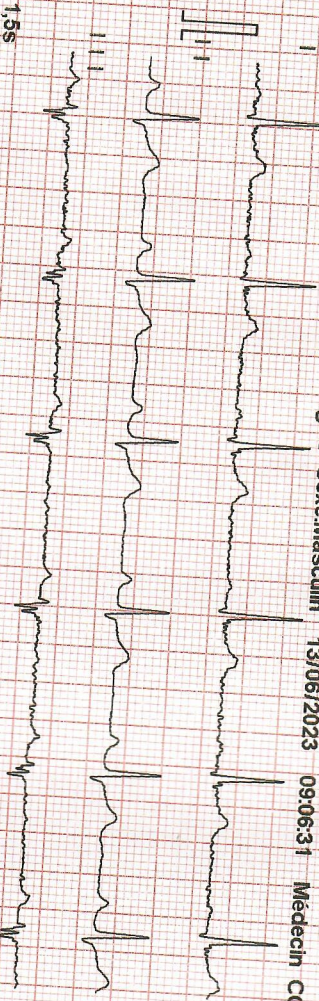

HR = 68

