



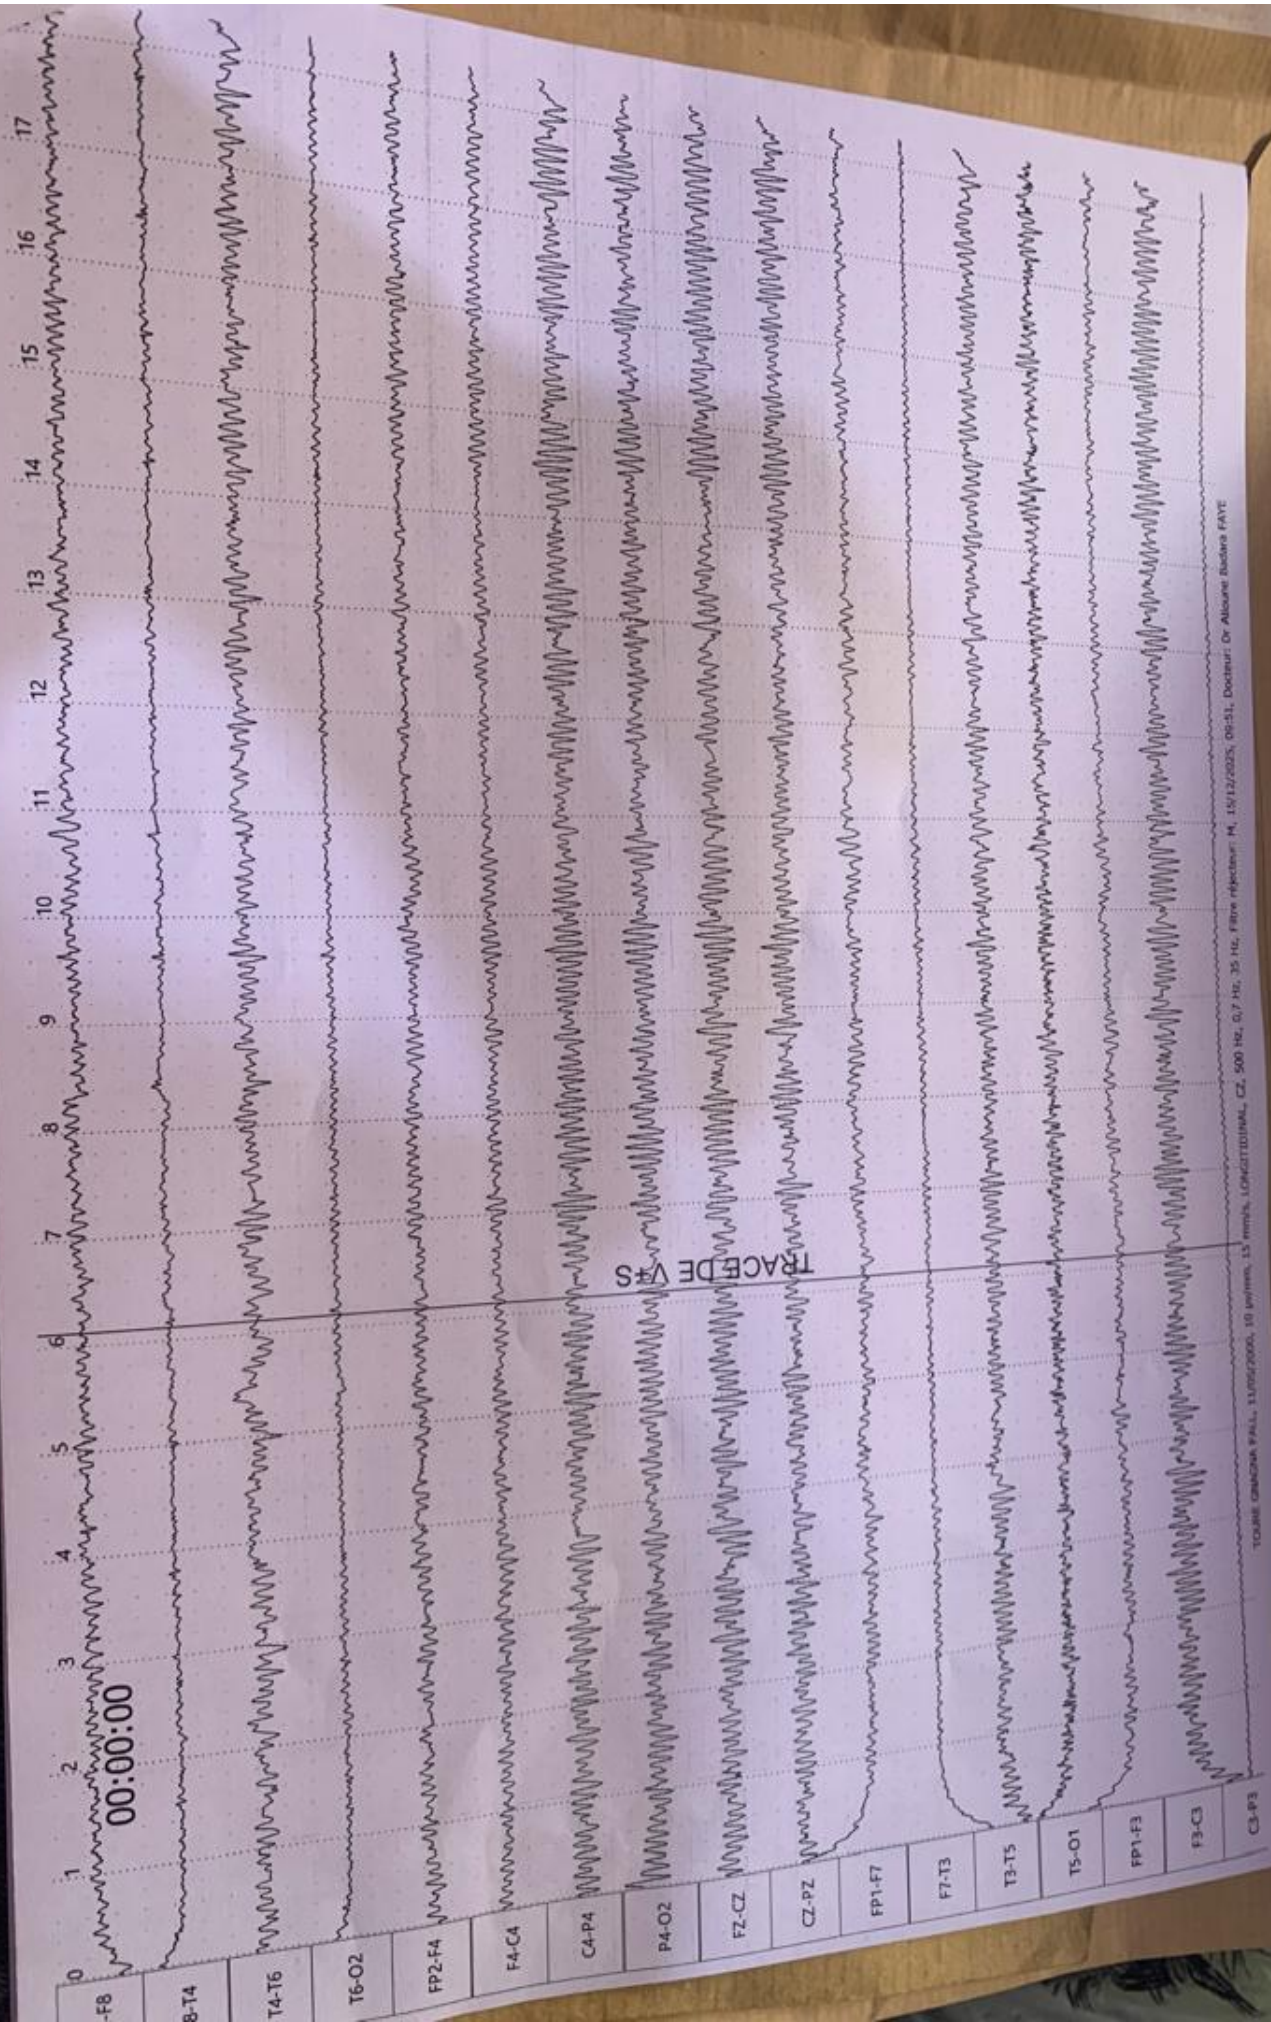


TOURNE CRANIOGRAPHY FALL, 11/05/2000, 10 minutes, 13 minutes, LONGITUDINAL, CZ, 500 Hz, 0.7 Hz, 35 Hz, Filter rejection: M, 15/12/2025, 00:51, Doodhuri Dr Alkumar Nadima FAYE


C3-P3

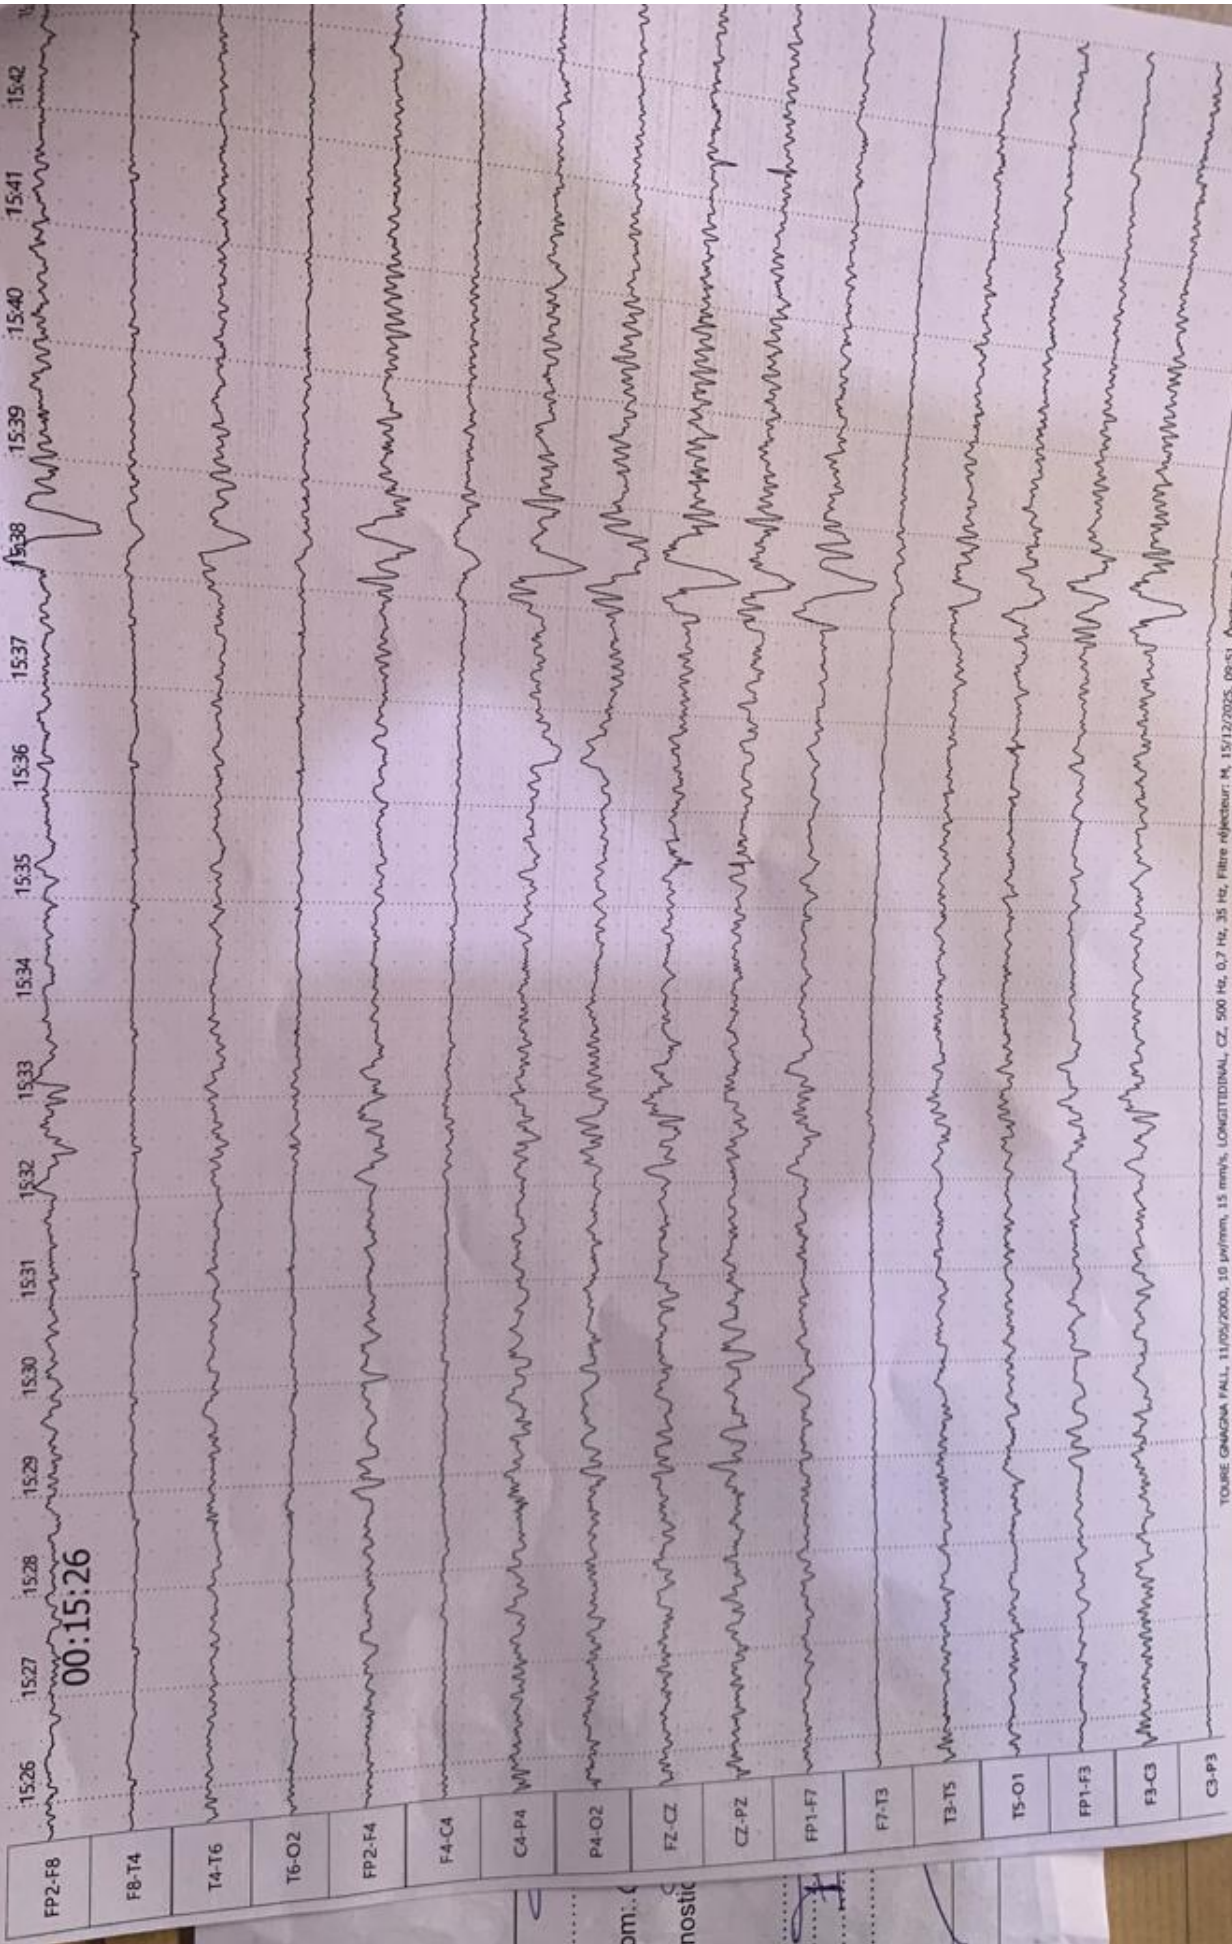

Nom:.....
Prénom:.....
Diagnostic:.....

3052 3053 3054 3055 3056 3057 3058 3100 3101 3102 3103 3104 3105 3106 3107 3108
00:30:51

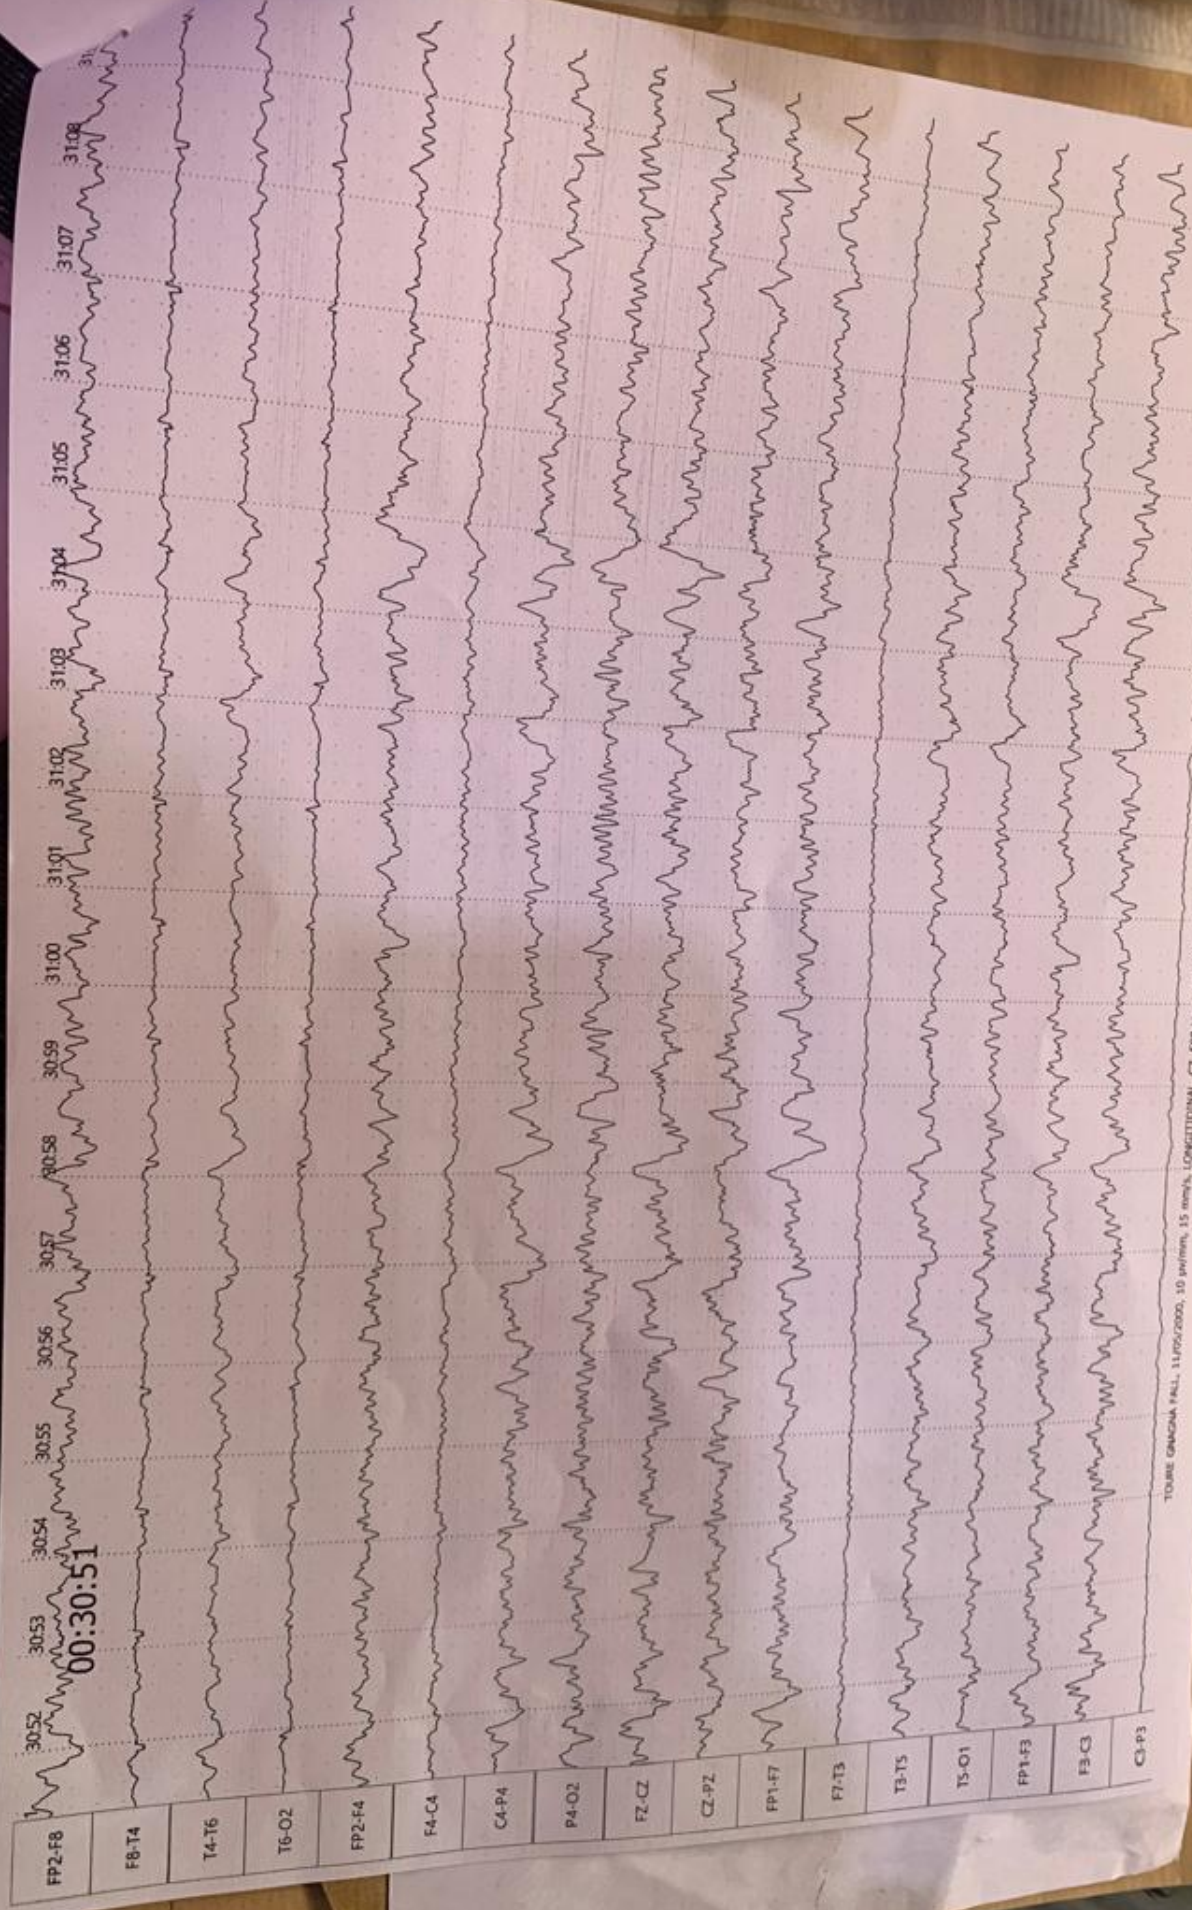

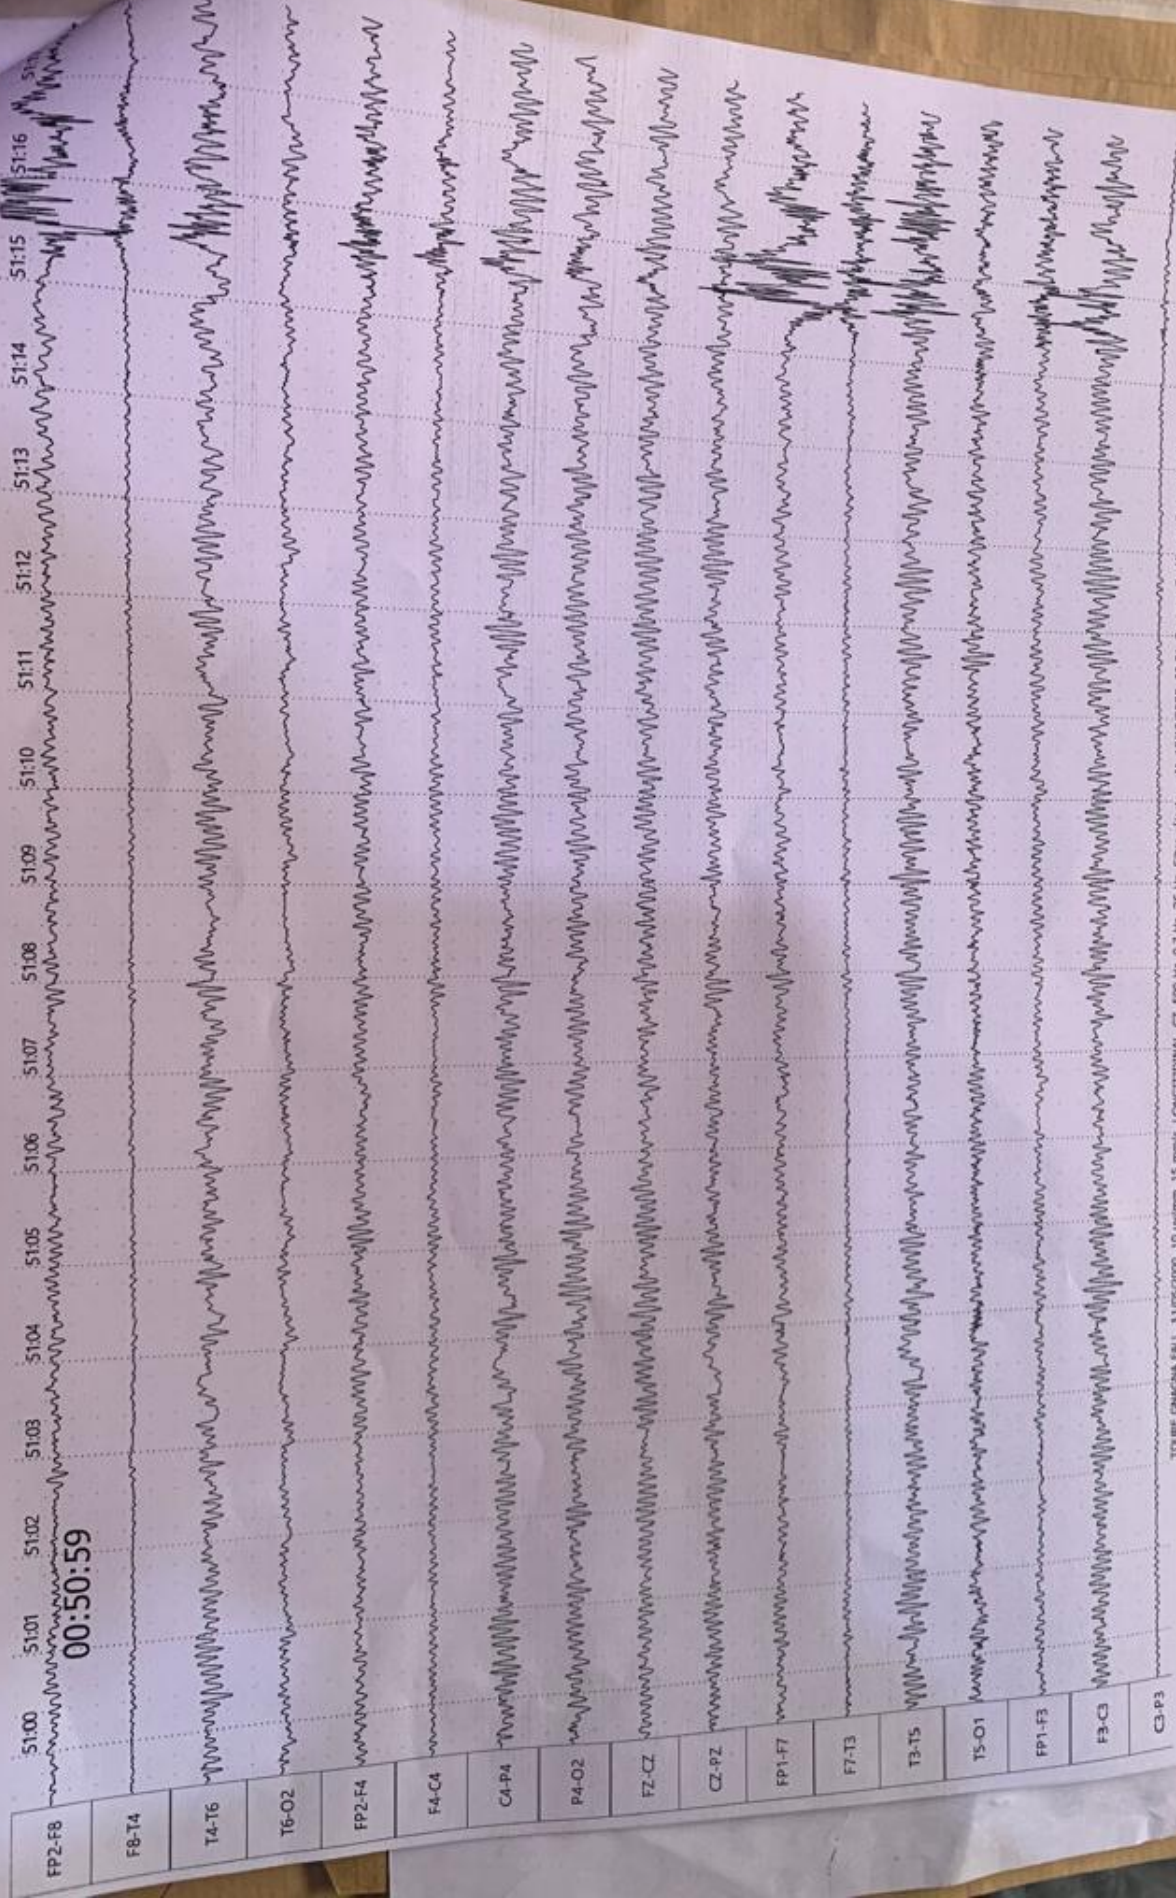

TOURNE OMAGNA FALL 1.1/05/2000, 10 µV/mm, 15 mm/s, LONGITUDINAL, CZ, 500 Hz, 0.7 Hz, 35 Hz, F8re réducteur M, 15/12/2023, 09:51, Dodeur: Dr. Alouane Badaro FAYE